



301 Patents; 60 invention patents; Exported to 133 countries

Choice of Millions of Dentists Worldwide

DTE

Scan and Login website
for more information



Since **1989**

CATALOGUE

Add: Information Industrial Park, National High-Tech Zone,
Guilin, Guangxi, 541004 P. R. China
Tel: Europe Sales Dept.: +86-773-5873196, +86-773-2125222
North America, South America &
Oceania Sales Dept.: +86-773-5873198, +86-773-2125123
Asia & Africa Sales Dept.: +86-773-5855350, +86-773-2125896
Fax: +86-773-5822450
E-mail: woodpecker@glwoodpecker.com, sales@glwoodpecker.com
Web: <http://www.glwoodpecker.com>



MedNet GmbH
Borkstrasse 10 · 48163 Muenster · Germany

2018 2.0 Edition

GUILIN WOODPECKER MEDICAL INSTRUMENT CO., LTD.



DTE

National high-tech enterprise

Choice of millions of dentists worldwide

Owner&CEO
Wu Xunxian



我是一个中国人，我会用我的一生
做好一件事，一件能让外国尊重，能让中
国人自豪的事。
吴勋勋 2006.2.19.

Introduction of Woodpecker Company

Concentration

Since **1989**, Woodpecker concentrates on the R&D of dental products.
7 product categories, **85%** domestic market share, and exported to **133** countries.

Innovation

306 employees, **75%** of them are Graduates or above or above,
18.6% are full time R&D team, **301** Intellectual rights, **60** invention patents.

Scale

26841m² existing manufacturing and research base, **80000**m² base under construction.
27 million USD invested to build up full-automatic processing and testing center.



Aerial View of Company



Science Building



Library




Lecture Hall



Show Room



Woodpecker products have been exported to 133 countries around the world

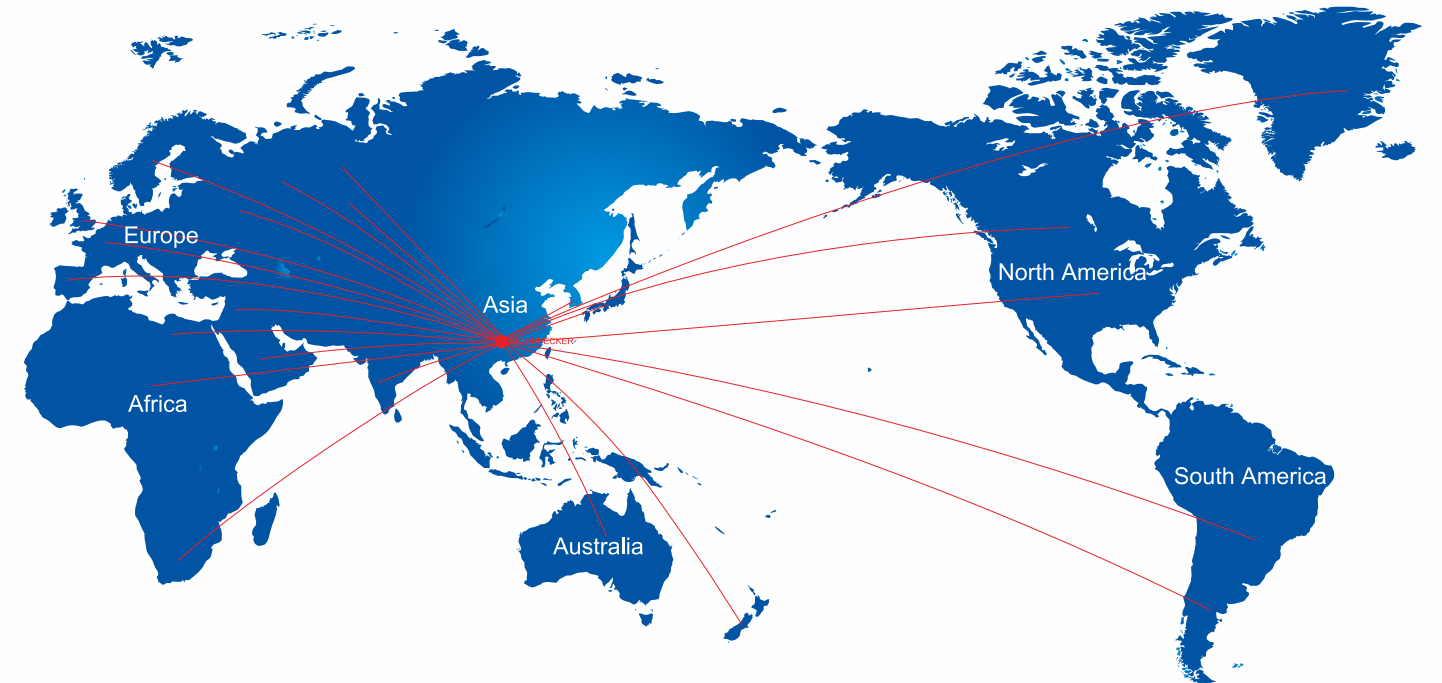

Europe 41 countries

Albania
Belarus
Finland
Ireland
Bulgaria
Netherlands
Estonia
Belgium
Montenegro
Andorra
Bosnia and Herzegovina
Croatia
Austria

Oceania 3 countries

Australia
New Caledonia
New Zealand

Poland
Lithuania
Denmark
German
Luxembourg
Russia
France
Romania
Czech
Latvia
Malta
Macedonia
Moldova
Norway
Portuguese

Sweden
Swiss
Serbia
Slovak
Slovenia
Ukraine
Spain
Greece
Hungary
Italy
Britain
Cyprus
Monaco

Asia 43 countries

Afghanistan
Bahrain
The United Arab Emirates
North Korea
Oman
Philippines
Azerbaijan
Georgia
Pakistan
South Korea
Kyrgyzstan
Cambodia
Qatar
Kuwait
Laos
Lebanon

Malaysia
Bengal
Myanmar
Nepal
Japan
Saudi Arabia
Sri Lanka
Tajikistan
Thailand
Turkey
Singapore
Syria
Armenia
Yemen
Iraq
Iran
Israel
India

Indonesia
Jordan
Vietnam
Mongolia
Uzbekistan
Turkmenistan
Maldives

America 22 countries

Canada
Nicaragua
USA
Salvador
Argentina
Guatemala
Paraguay
Venezuela
Panama
Uruguay
Brazil
Chile
Bolivia
Cuba
Dominican
Puerto Rico

Ecuador
Costa Rica
Colombia
Honduras
Peru
Mexico

Africa 24 countries

Algeria
Libya
Senegal
Egypt
Reunion
Sudan
Ghana
Madagascar
Botswana
Zimbabwe
Morocco
Burkina Faso
Cameroon
Namibia
Mozambique

Kenya
South Africa
Ethiopia
Mauritius
Nigeria
Niger
Tunisia
Zambia
Somalia

All staffs of Woodpecker




29 years' technical innovation

Made in China German quality
High – quality Durable Innovative

Experienced R&D team in dental instrument industry


Constituted of 11 teams specializing on each products in Woodpecker. Woodpecker now has 60 professional engineers focusing on researching and development of new technique in dental industry . And our target is to satisfy our customers by producing innovative and safe products
Professional R&D team for each product.
29 years' concentration and innovation in core technology research and development.

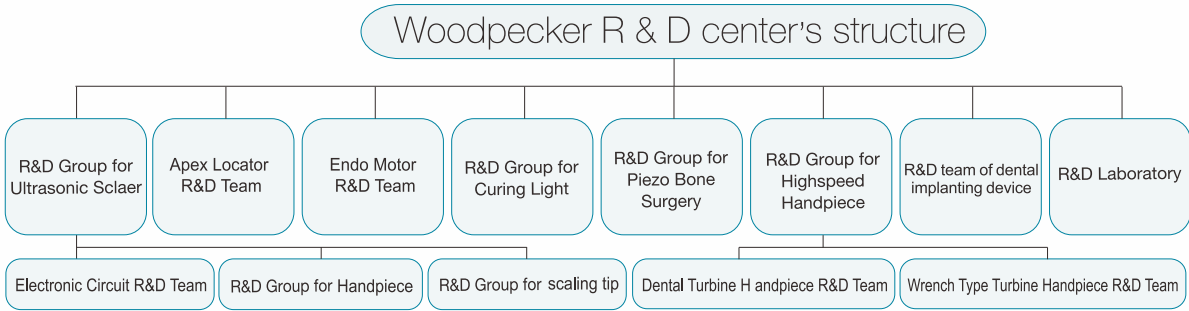


Advanced processing equipment in dental industry



The processing of core parts in handpiece

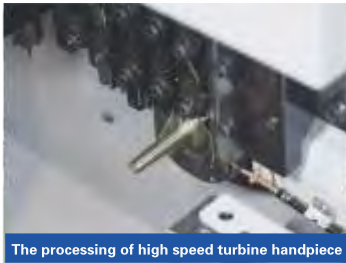

The processing of high speed turbine handpiece


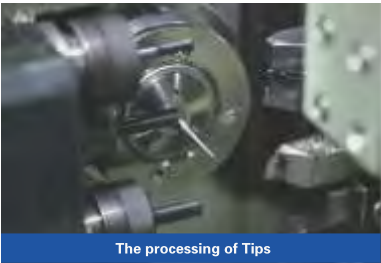


The processing of Tips

- Invest 21.3 million USD to the construction of CNC Center which occupies an area of 2300 m². Automatic processing equipment is imported from Japan.
- The production of every core part is supported by equipment which costs more than a million yuan.

Leading laboratory in dental industry

Occupy an area of 1280 m².
Imported professional equipment from Germany, U.S.A, and Japan costs 5.7 million USD.

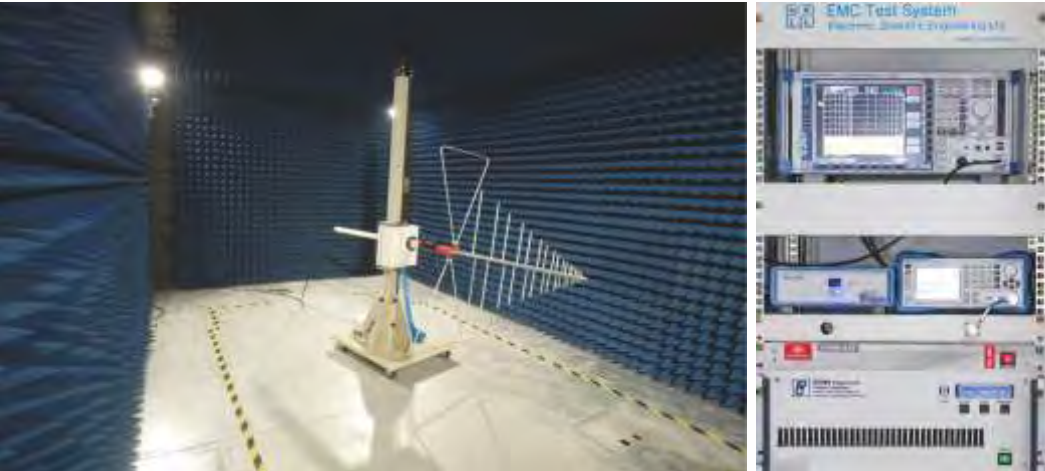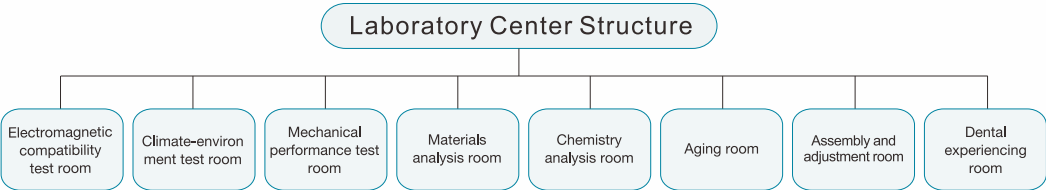

EMC Tester system The only EMC Test System in Chinese dental industry which costs 0.76 million USD.



Mechanical Environmental Laboratory Simulate various extremely mechanical environments to ensure the quality of products.



Climate Environmental Laboratory Simulate various extreme climate environments to ensure the quality of products.



Direct reading spectrometer imported from Germany, to detect components of elements, improving quality of raw material



Roundness measuring instrument imported from Japan, high degree of accuracy(0.01um)



Roughness detector imported from Japan, to test the roughness of metal surface




Energy dispersive X-ray fluorescence spectrometer To detect the harmful materials, according to the demand of EU standard

How to check Authenticity



*The new anti-forgery query system is only applicable to products produced since 11st, September, 2014.

Harm of fake products

 and **DTE** are two brands of Guilin Woodpecker Medical Instrument Co., Ltd. Recently, there are many fake ultrasonic scaler handpieces, tips and curing lights are produced and sold into the market, which does harm to users' interest. On this issue, Woodpecker will crack down fake products and provide safe and secure medical instrument products.

1. Harm of fake ultrasonic scaler handpieces.

- 1.1 Fake handpieces with poor-designed inner structure can lead to frequent power leakage, which may cause medical accidents.
- 1.2 Material used on fake handpieces don't pass biocompatible test, which can easily lead to irritability and poisoning.
- 1.3 Fake handpieces have quality problems of overheating, non-vibration and cracking, which cause ultrasonic scalers out of order.
- 1.4 Fake handpieces can't be compatible with ultrasonic scalers, thus leading to circuit burn out.

2. Harm of fake scaler tips.

- 2.1 Fake tips are low in toughness, poor in resistance and easy to crack, thus easily cause medical accident.
- 2.2 Fake tips' screw threads are roughly processed, which can cause handpiece's screw loosening and cracking.
- 2.3 Material used on fake tips is inferior and easily rusting, which can cause infection of patient.
- 2.4 Fake tips have problem of poor water-spraying, bad screw-thread fit and water leaking, which leads ultrasonic scalers work wrongly.

3. Harm of fake curing light.

- 3.1 Fake curing light's batteries can cause self-ignite, even explosion with poor-quality material and no complete charging management
- 3.2 Light intensity of fake curing light is not constant, when battery level goes down under 60%, it would lead to incomplete solidification of resin, causing secondary dental caries.

CONTENTS

DTE	New Arrivals	1-10
	Implante-X	1-2
	Lx16	3-4
	Piezoelectric Ceramics Painless Periodontal	5-10
DTE	Ultrasonic Scaler	11-21
	D600	11-12
	S6	13-14
	D7 LED D5 LED D3 LED D2 LED	15-16
	D1 D6 LED Built-in Scaler	17-18
	Tips advantage	19
DTE	Apex Locator	20-24
	DPEX III Golden Standard	20
	DPEX III DPEX I	21-22
	MINIPEX	23-24
DTE	Endo Motor	25-30
	E-COM	25-28
	Endo Smart	29-30
DTE	Curing light	31-40
	X-Cure	31-32
	B-Cure	33-34
	ILED	35-36
	LUX E LUX V MINI S	37-38
	LUX VI LUX I	39
	LED.H ORTHO	40
DTE	Dental Turbine Handpiece	41-44
	Dental Handpieces'Advantages	41-42
	Models of Dental Handpieces	43-44
DTE	Bone Piezo Surgery	45-48
	Surgery X	45-46
	DS-II LED	47-48
DTE	Tips	49-51
	Comparison of Scaler Tips	49-51
	Function of Scaler Tips	52-59

	Spare Parts	60-62

New Arrivals

Ultrasonic
Scaler

Apex Locator

Endo Motor

Curing light

Dental Turbine
Handpiece

Ultrasonrgery

Tips

Implant-X

Precise toision Srtrong and powerful

Woodpecker Implant Motor adopts mute motor imported from Swiss. Advanced FOC controlling technique blends low speed performance with high speed performance. In order to verify the clinical features of flexible response and stable safety, Implant Motor R & D personnel go into the operating room, getting them involved in clinical applications. Under the instruction and assistance of experts from home and abroad, they finally complete the clinical optimization of product. Woodpecker spares no efforts to provide you high quality products.

Rapid and stable response of mute motor

Light motor, more flexible operation

Large-size touching screen, clear display

Strong twist force; accurate limited force

Low speed thread tapping; safer constant speed



LX16

A New Generation Of High Power Dental Diode Lasers

Laser parameter:

- Wavelengths & optical power:

976 \pm 10 nm / approx. 0.1 – 10.0 W (CW), optical peak power approx. 16 W;

650 \pm 10 nm / approx. 25 – 200 mW (CW)

- Laser system:

976 nm: Class IV; 650 nm: Class II (according to IEC 60825-1)

- Emission modes:

CW (continuous wave), chopped 1 Hz to 50 kHz

Aiming beam:

650 \pm 10 nm / 1 – 3 mW (CW)

- Optical fiber thickness:

320 and 200 μ m (fiber tips), 8 mm (glass rods)

- Battery:

5200mAh@11.1V(57.7Wh)



WORLDWIDE LAUNCHING — *PT 3*

PIEZOELECTRIC CERAMICS PAINLESS PERIODONTAL TREATMENT DEVICE

18 invention patents **116** national patents
29 years of research on ultrasonic scaling

PT 3 main specifications:

Frequency: 28000Hz

Tips hardness: 30HRC

Vibration amplitude: 20~60um

Treatment depth: 14mm

Equipped with: 2 handpieces+10 tips

Treatment effect:



Before treatment



Under treatment



After treatment



One month later

Save scaling

Tip amplitude is about 20~60 μm, equivalently third of diameter of a single hair.
 Excellent sci-tech outcome assures your save and painless treatment



Implant maintenance P90

Tip end is wrapped with PEEK material
 Clean and repair implants



PT 5

PAINLESS PERIODONTAL

Piezoelectric Ceramics Painless
Periodontal Treatment Device



Root canal treatment



ENDO SCALING FAST & COMPLETE



After scaling, there is no smear layer on root canal surface, only a few amount of debris left.

Endo scaling
(E51 E52)




For removing the calcification
and bad fillings in root canal
(E3D)



For removing the
calcification in the coronal
third of the root canal
(P4D)



Looking for root canal orifice
(E12D)



Diamond-coated, ball head,
for looking for root canal
orifice with security,
accuracy and efficiency

Root canal retreatment,
removing foreign body
(E6 E7 E14 E15)



Special material (E6, E7),
extremely thin and soft,
good conductivity to ultrasound


Main specifications:

Frequency: 28000Hz — 42000Hz

Vibration amplitude: 20~60um

Tips hardness: 30HRC

Treatment depth: 14mm

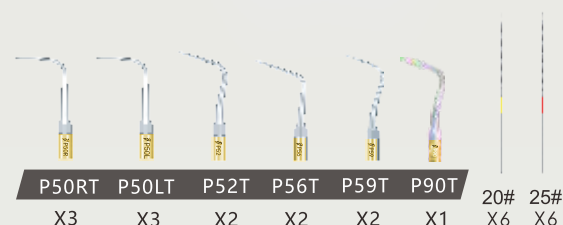


Elliptical vibration track endows polishing function.

Tip amplitude is about 20~60 μ m, equivalently third of diameter of a single hair.

Elliptical vibration track disperses the impact force between tip and teeth while realizing 360° scaling and polishing.

Perform scaling and polishing at the same time.

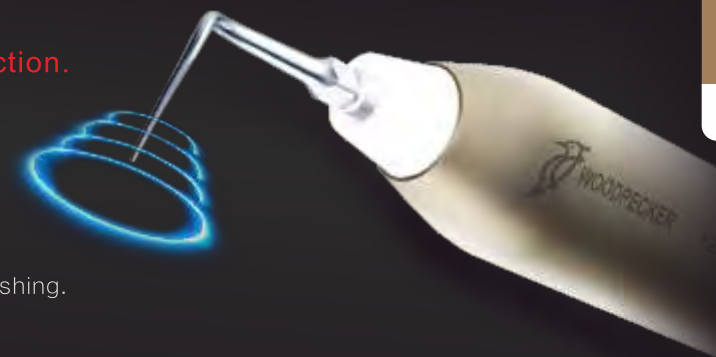

Distinctive touching system

Clear control panel.

12 grades power setting

Optional dual water supply modes: external water supply & automatic water supply

Ultra-sensitive touching system

Stickers, gloves, and drippings will not affect operation.



Sealed handpiece with LED ensures clear oral cavity vision

Handpiece can be autoclaved,
avoiding cross-infection
Durable life span



E51



120° angle holder: Swishing anterior teeth coordinated with swished file after root canal preparation, used in E mode.

E52



95° angle holder: Swishing posterior teeth coordinated with swished file after root canal preparation, used in E mode.

E3



Using ultrasonic melt to press gutta-percha for lateral pressure, used in E mode without water.

E3D



Diamond-coated(40µm) instrument for removing calcification and bad filling material in root canal, used in E mode.

E6



Special material

Thin and flexible, used for removing foreign body in deep cannal.

E7



Special material

Thin and flexible, used for removing foreign body in 1/3 cannal.

P4D



Diamond coated(40µm), used to remove the calcification in the coronal third of the root canal and used in E mode.

P50L



Used for subgingival scaling, periodontal pocket probing and root planing

Applicable areas: labial proximal surface of upper front teeth, lingual proximal surface of upper front teeth, buccal interproximal in B quadrant, and lingual interproximal in C quadrant

P50R



Used for subgingival scaling, periodontal pocket probing and root planing

Applicable areas: labial proximal surface of upper front teeth, lingual proximal surface of upper front teeth, lingual interproxima in B quadrant

P52



Used for subgingival scaling, periodontal pocket probing and root planing

Applicable areas: lingual and lip side of front teeth and lower front teeth, buccal side in A quadrant and maxillofacial side in B quadrant

P53L



Used for subgingival scaling, periodontal pocket probing and root planing

Applicable areas: labial proximal surface of upper front teeth, lingual proximal surface of upper front teeth, buccal interproximal in B quadrant, and lingual interproximal in C quadrant

P53R



Used for subgingival scaling, periodontal pocket probing and root planing

Applicable areas: labial proximal surface of upper front teeth, lingual proximal surface of upper front teeth, lingual interproximal in B quadrant

P56



Use for removing big calculus, no hurt to gum when scaling in the gingival margin

Applicable areas: lingual and lip side of Front teeth and lower front teeth, buccal side in A quadrant and maxillofacial side in B quadrant

P59



Use for subgingival scaling, periodontal pocket probing and root planing

Applicable areas: lingual and lip side of front teeth and lower front teeth, buccal side in A quadrant and maxillofacial side in B quadrant

P90



Implant maintenance

Clean implants and restorations

Make sure water can reach the top of tip.

Power should be no more than level 7, or the peek head may be broken

SPOILING YOU SO MUCH !



D600 Ultrasonic Scaler

Intelligent power output Experience painless treatment

29 years innovation

Professional scaler manufacturers

Woodpecker scaler owns **103** national patents **9** national invention patents



Supragingival scaling

Subgingival scaling

Endodontic irrigation



Endodontic irrigation



After ultrasonic irrigation, there is no smear layer on surface but a few amount of dentin debris in the root canal.


Root canal irrigation is the most widely used clinical support methods. Its purpose is to remove the substance inside root canal, dissolve diseased tissue, remove pathogenic microorganisms, and remove smear layer. Lubricate the root canal internal wall. During root canal preparation process, prevent the infectious substance from being pushed to the deep part or out of the apical foramen, reducing the risk of instrument fracture in root canal.

Compared with the traditional syringe irrigation, ultrasonic irrigation can better remove bacteria, dentin debris, and smear layer in root canal. And it can well clean special structures such as the lateral branch canal and root canal narrow area. Currently, ultrasonic irrigation is widely used in endodontic therapy in order to receive a better root canal preparation effect.

Sine wave drive

Avoid pain caused by power surge; ensuring comfortable treatment.

D600 Mild power output




Intelligent touching system

Clear control panel

Ultra-sensitive

Waterproof design



Automatic water supply system

Easy to change water, eliminating redundant steps

Hydrogen peroxide, sodium hypochlorite, and chlorhexidine is available

Clear 50ml scale mark makes it convenient for formulating liquid



Detachable handpiece with light

Detachable handpiece with light

Detachable handpiece with light enables better visibility

and adopts new sealing technique, bringing patients comfortable scaling.

High-quality handpiece

Aluminum shell can be autoclaved, causing no cracking or deformation

Advanced handpiece sealing technique enables long durability

User-friendly design brings better holding feeling



D600 Ultrasonic Scaler is equipped with various shapes of tips, including slender tip which is specially used to perform subgingival scaling. Operators can choose tip according to the size and position of dental calculus. While tip starts to vibrating, the water spraying system should spray water to tip to form water spray at the same time.

On the one hand, it can cool the tip. On the other hand, it will help form cavitation effect, that is, subtle vacuum bubble quickly collapses and produces energy to scour the calculus, plaque and the broken tartar and blood.

S6

Ultrasonic Endodontic Expert

Ultrasonic
Scaler

13

Ultrasonic
Scaler

14

Comfortable Scaling

Integrate supragingival scaling, subgingival scaling,
and endodontic treatment into a whole

Microcomputer control and automatic frequency
tracking enable more stable performance

Intelligent degenerative system enhances professional operation

Smart touching system makes it easier to operate


Main unit input: -24v 50hz

Water pressure: 0.01MPa-0.5MPa

Frequency: 28KHZ+ 3KHZ

Main unit weight: 650g

Dimensions: 197mmx174mmx74mm

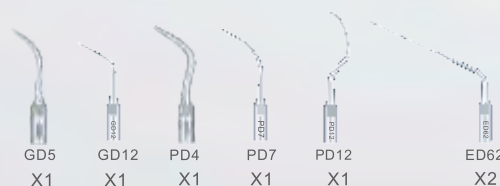

D7-LED

Use of anti-rot material in internal water system enables use of clinical solutions such as hydrogen peroxide, sodium hypochlorite, and chlorhexidine, improving the effect of periodontal treatment and endodontic irrigation dramatically. Detachable handpiece enables better visibility and adopts new sealing technique, bringing patients comfortable scaling. Automatic degenerative feedback and constant power output brings rather comfortable scaling.

- Scaling
- Perio
- Endo
- Handpiece with LED
- Auto-water supply

Voltage input: ~220V 50HZ
Main unit weight: 1.17kg
Main unit input: ~24V 50HZ 1.3A
Transformer weight: 1.0kg
Output power: 38VA
Frequency: 28kHz ± 3KHz
Dimensions: 241mmX193mmX97mm

Expert in endodontic irrigation



Clear vision



Blurred vision




D5-LED

- Scaling
- Perio
- Endo
- Handpiece with LED

Detachable handpiece with light enables better visibility. Handpiece adopts new sealing technique, bringing patients comfortable scaling. Automatic degenerative feedback and constant power output brings rather comfortable scaling.

Voltage input: ~220V 50Hz
Main unit input: ~24V 50Hz 1.3A
Output power: 38VA
Frequency: 28kHz ± 3kHz
Water pressure: 0.1bar~5bar (0.01MPa~0.5MPa)
Main unit weight: 0.65kg
Transformer weight: 1kg
Dimensions: 188mm × 159mm × 81mm

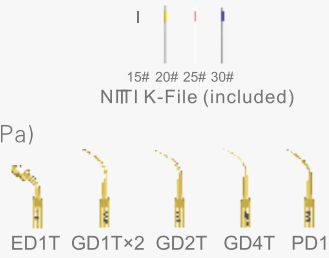


D3-LED

- Scaling
- Perio
- Handpiece with LED

Detachable handpiece with light enables better visibility. Microcomputer control, automatic frequency tracking. Automatic degenerative feedback and constant power output brings rather comfortable scaling.

Voltage input: ~220V 50Hz
Main unit input: ~24V 50Hz 1.3A
Output power: 38VA
Frequency: 28kHz ± 3kHz
Water pressure: 0.1bar~5bar (0.01MPa~0.5MPa)
Main unit weight: 0.66kg
Transformer weight: 1kg
Dimensions: 198mm × 134mm × 80mm




D2-LED

- Scaling
- Perio
- Handpiece with LED

Built-in power supply; automatic frequency tracking system enables stable performance. Microcomputer control; easy and high efficiency operation. Silicone sleeve of handpiece can be autoclaved to avoid cross-infection.

Voltage input: ~220V 50Hz
Output power: 38VA
Frequency: 28kHz ± 3kHz
Water pressure: 0.1bar~5bar (0.01MPa~0.5MPa)
Main unit weight: 1.56kg
Dimensions: 227mm × 158mm × 75mm





D1

Scaling Perio

Sealed handpiece
Automatic frequency tracking system
Automatic degenerative feedback and constant power output brings rather comfortable scaling.

Voltage input: ~220V 50Hz
Main unit input: ~24V 50Hz 1.3A
Output power: 38VA
Frequency: 28kHz ± 3kHz
Water pressure: 0.1bar~5bar (0.01MPa~0.5MPa)
Main unit weight: 0.62kg
Transformer weight: 1kg
Dimensions: 203mm × 138mm × 94mm





D6-LED

Automatic water supply system brings more convenient operation. (Optional)
Detachable handpiece with light enables better visibility. Automatic degenerative feedback and constant power output brings more comfortable scaling.

Scaling Perio Endo Handpiece with LED Auto-water supply


Voltage input: 220 – 240V~ 50Hz/60Hz 150mA
Main unit input: 24V~ 50Hz/60Hz 1.3A
Output power: 5V~ 50Hz/60Hz 200mA
Frequency: 3W~20W
Water pressure: 28kHz ± 3kHz
Main unit weight: 0.1bar~5bar (0.01MPa~0.5MPa)
Transformer weight: 1kg
Dimensions: 193.5mm × 133mm × 75.8mm

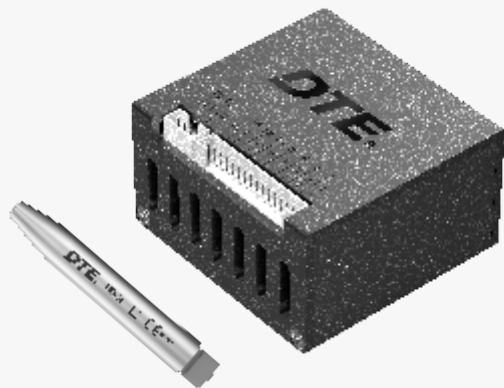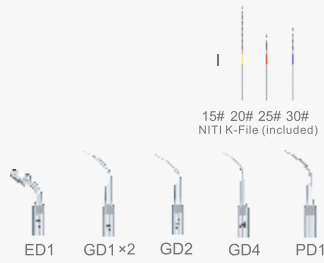

V6 LED

Main unit input: ~24V50HZ
Main unit weight: 0.13kg
Output power: 38VA
Frequency: 28KHz±3KHz
Dimensions: 59mm×57mm×33mm

Supragingival & Subgingival scaling
Optional Endo function
Detachable metal handpiece prevents crack
Microcomputer control, automatic frequency tracking
30% smaller than the volume of N2,
occupies less space of tray in dental chair

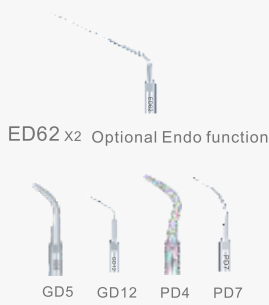


V3 LED

Detachable handpiece with light
Integrate scaling, Endo, and Perio function into a whole.
Microcomputer control and automatic frequency tracking
Automatic degenerative feedback and constant power output brings more comfortable scaling.

Main unit input: ~24V 50Hz
Output power: 38VA
Frequency: 28kHz ± 3kHz
Water pressure: 0.1bar~5bar (0.01MPa~0.5MPa)
Main unit weight: 0.2kg
Dimensions: 74mm × 56mm × 38mm

V3 Match detachable handpiece HD – 7H
V3 LED Match detachable handpiece HD – 7L

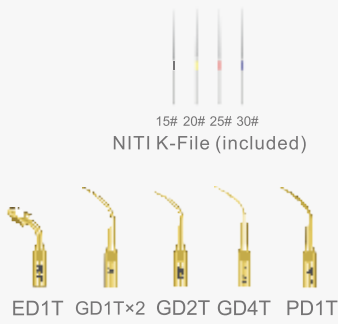


V2 LED

Detachable handpiece with light
Microcomputer control and automatic frequency tracking
Automatic degenerative feedback and constant power output brings more comfortable scaling.

Main unit input: ~24V 50Hz
Output power: 38VA
Frequency: 28kHz ± 3kHz
Water pressure: 0.1bar~5bar (0.01MPa~0.5MPa)
Main unit weight: 0.2kg
Dimensions: 74mm × 56mm × 38mm

V2 Match detachable handpiece HD – 7H
V2 LED Match detachable handpiece HD – 7L

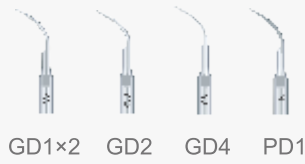


V1

Sealed handpiece;
Microcomputer control and automatic frequency tracking
Automatic degenerative feedback and constant power output brings rather comfortable scaling.

Main unit input: ~24V 50Hz
Output power: 38VA
Frequency: 30kHz ± 3kHz
Water pressure: 0.1bar~5bar (0.01MPa~0.5MPa)
Main unit weight: 0.2kg
Dimensions: 74mm × 56mm × 38mm

V1 Match detachable handpiece HD – 7L

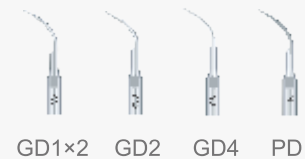

Compatibility of tip

The working frequency range of Swiss E brand: <32000Hz



Woodpecker tip can perfectly match E brand scaler

Compatibility of handpiece

Woodpecker: Resonant frequency 29.263KHz E brand: Resonant frequency 29.263KHz




Technical data of Woodpecker handpiece is the same as that of E brand.
Handpiece of both brands can be exchanged.

Smooth tip does no harm to teeth.

Select high-quality medical material which is durable and wear-resistant.
Adopt advanced laser drilling technology and experience 35 strict production processes as well as 5 inspections.

The picture shows the image of tips after a 160 times magnification.

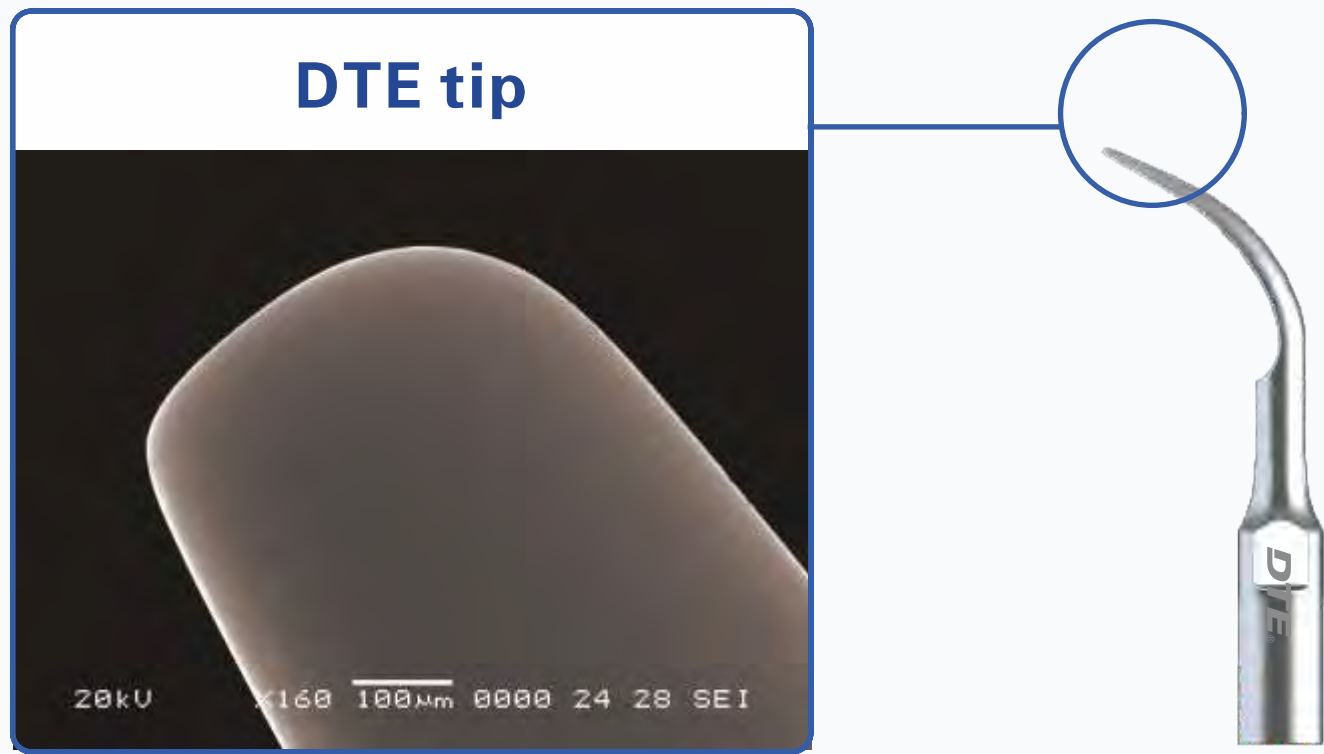

APEX LOCATOR
DPEX III GOLDEN STANDARD
25 National Patents 8 Invention Patents



Clinical data matching,
The accuracy rate has been improved to

97.71%

DPEX III

- LCD screen, the trajectory of the file can be clearly shown with different colors.
- Multi-frequency apical positioning technology, avoiding the influence of subjective factors for measurement results.
- Measurement results will not be affected by tooth type, root canal internal environment.
- Rechargeable lithium battery.
- Adjustable viewing angle.

DPEX I

- Clear Image.
- Multi-frequency apical positioning technology, avoiding the influence of subjective factors for measurement results.
- Adjustable viewing angle.



Battery 3.7V/750mAh
 Power consumption ≤0.5W
 Screen 4.5"LCD
 Main unit weight 385g
 Dimensions 138mm×77mm×107mm

Industrial design patent No.:CN 201130378913.4



Battery 3 piecesAAA alkaline batteries
 Power consumption ≤0.3W
 Screen 4.9"LCD
 Main unit weight 395g
 Dimensions 105mm×142mm×40mm

Industrial design patent No.:CN 201130378728.5

Minipex Apex Locator

COMBINATION OF TECHNIQUE AND ART

QUALITY AND BEAUTY COEXIST

Small size
High precision

Simplicity and Elegance

Back-up ring design
Multi-angle adjustment
Arbitrary set, measure as wishes
Lightweight, easy to take
Outstanding authentic quality

Light but Powerful

A total weight of merely 71g
Dimension: 70mm × 62mm × 20mm
With superb technique
100% automatic digital calibration
Light body together with stable performance



Voice Prompt

Multi – frequency independent network measuring technique, enlarging the apical narrow area
Double assurance to accurate measurement
Alarm rings when the distance between root canal needle and root canal is less than 2 mm
Providing effective protection to both dentists and patients

Simplified Body Design with High Sensitivity

Clinical data fitting
Measurement accuracy up to 97.71%
Updated chip, real-time response, double sensibility
Innovative algorithm, intelligent anti – interference

E-COM

PRESET VARIOUS FILE SYSTEMS



Preset various file systems so that the dentist can directly choose the file system that they need, which brings dentists convenience while they need to use different kinds of files.



CUSTOMIZATION

Storage of 9 user-defined modes allows invocation at any time.
Under each mode, continuous motion, reciprocating motion, and reverse motion are for options.
Torque and speed is adjustable.

EFFECTIVELY PREVENT NEEDLE BREAKAGE



Adopt real-time feedback technology and dynamic torque control, realizing automatic reverse, effectively preventing fracture.





Cordless handpiece
Operation without
limit of cord



Six optional angles
More convenient treatment



All-angle OLED screen
Real-time dynamic
torque display



Fast handover between
Continuous Motion
Mode and Reciprocating
Motion Mode

COMBINED LENGTH DETERMINATION MODE

E-Master Pro can be connected to the matched Apex locator to realize apex locating function.

By connecting the E-Master to the matched Apex locator, the position of the file tip inside the canal can be monitored during the procedure and many automatic functions such as Auto Apical Reverse can be activated.



Maximum compatibility

Wide torque and speed range make it adapt to various file systems such as FKG, XP-endo, and Shaper in the market.

Recommended speed is 800–1000rpm.

Recommended maximum torque setting for Dentsply Protaper Gold is 5N.cm.



NIMBLE CONTRA-ANGLE

Contra-angle can be autoclaved to avoid cross-infection.

Adjustable angle make it available for different teeth positions.

Small and exquisite head provides unobstructed views.

IMPORTED MOTOR

15.5: 1 reduction ratio endows strong power and efficient cutting.

Durable planet gear gearbox prolongs service life of device.



Endo Smart

Effectively prevent file breakage


Adopt real-time feedback technology and dynamic torque control, realizing automatic reverse, effectively preventing fracture.

Customization

Storage of 9 user-defined modes allows invocation at any time.

Under each mode, continuous motion, reciprocating motion, and reverse motion are for options.

Torque and speed is adjustable

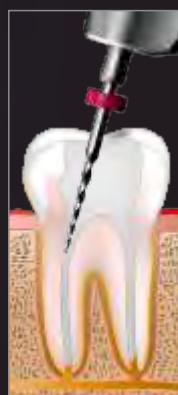

Maximum compatibility

Wide torque and speed range make it adapt to various file systems such as FKG, XP-endo, and Shaper in the market.

Recommended speed is 800-1000rpm.

Recommended maximum torque setting for Dentsply Protaper Gold is 5N.cm.



WIRELESS CHARGING

Non-contact, reliable

All-angle OLED screen

Without visual angle limit, clear display can be guaranteed even under strong light. Available display of speed, torque, and battery consumption

Nimble Contra-angle

Contra-angle can be autoclaved to avoid cross-infection. Adjustable angle make it available for different teeth positions. Small and exquisite head provides unobstructed views.

Imported Motor

15.5: 1

reduction ratio endows strong power and efficient cutting.

Durable planet gear gearbox prolongs service life of device.

ONECURE

X-Cure


Wide Spectrum Curing Light

Eleven years of Curing Light technological research and development
Wide Spectrum LED Curing Light X-Cure emerges at the right moment
Compared with general LED Curing Light, it is of wider emission wavelength range,
better curing bleaching resin and transparent resin.

Wide Spectrum Curing

Emission wavelength range of general Curing Light is 420nm - 480nm
Emission wavelength range of X-Cure wide spectrum Curing Light is 385nm - 515nm,
adding a new wave band of 385nm - 420nm.
The additional wave band can better curing resin materials containing
new-style photoinitiators such as TPO. For example,
restoration materials like Tetric N - Ceram Bulk Fill (Ivoclar),
Amelogen Plus (Ultradent), and ENA Hri (Micerium).
This new wave band can also reduce the risk of resin falling off and incomplete curing.

X-Cure Spectral Curve and Resin Spectral Absorptivity

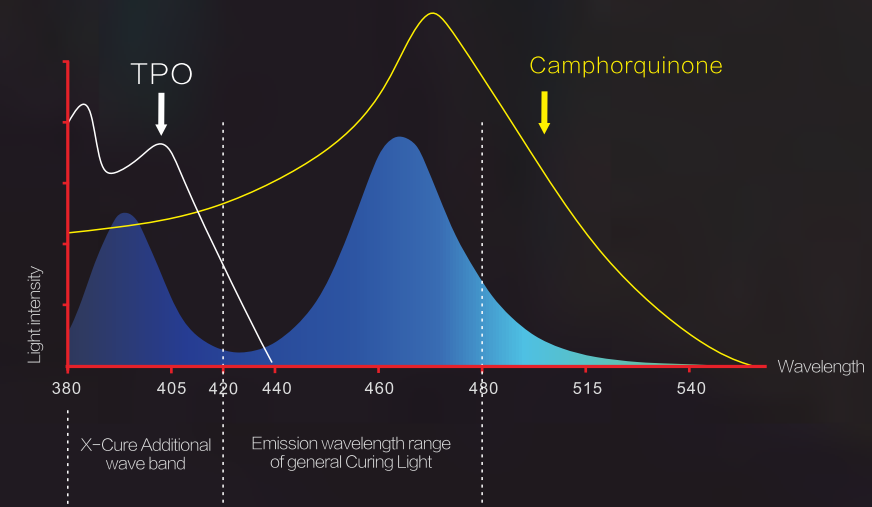

The light-absorbing peak of traditional material (including camphorquinone;
the yellow line on the figure) is 460nm,
so the curing can be done by either general Curing Light or Wide Spectrum Curing Light.
But camphorquinone is of a yellow color.
It is not suitable to add large amounts of it to bleaching resin or light-colored resins.

The light-absorbing peak of new materials (including TPO;
the white line in the figure above) is 405nm.
Compared with general LED Curing Light,
X-Cure owns additional 385nm - 420nm wave band which is able
to better curing this kind of new material. TPO is of white color.
Thus it is suitable for adding to the bleaching resin and light-colored resin.



B-cure

Broad-spectrum LED Curing Light

More human-friendly design

B-Cure adopts ergonomic design with smooth lines and small size. Doctors can easily hold it.

3 seconds for curing

B-Cure is equipped with 5w LED. The maximum light intensity can reach 2000mw/cm² with such a small size.


Curing normal resin that is thicker than 2mm in three seconds. Play an important role in cementation of all-ceramic restoration and orthodontic bracket.

Ortho mode

In the orthodontics mode that is unique to B-Cure, the light intensity automatically adjusts to 2000mw/cm².

The user can set the single curing time for 3s or 5s, and the device will automatically conduct 10 circles of curing with interval of 1s.

One operation can basically finish the cementation of 2 to 3 bracket, which reduce operations and improves efficiency.

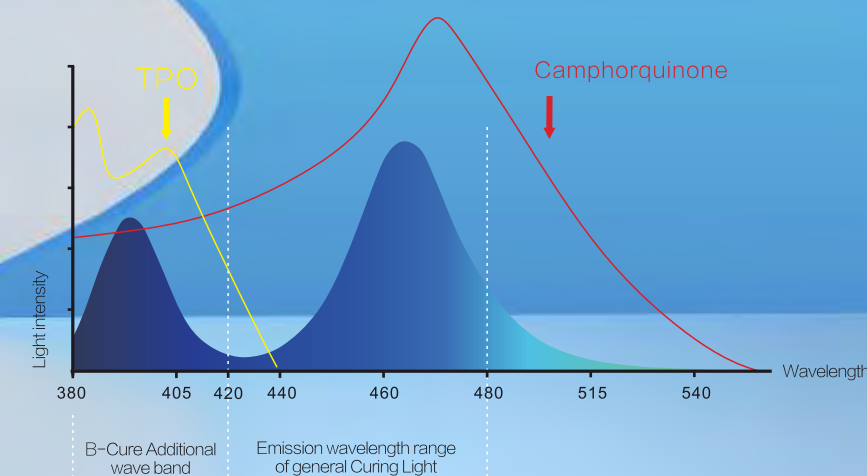

CURING LIGHT

iLed



1
SEC

Cure 2mm resins in one second

light intensity up to **2300** mw/cm²

1SEC

FOR CURING

Go quicker than ever



CONSTANT POWER OUTPUT
Born for restoration

1 SEC FOR CURING
Go quicker than ever

360°ROTATABLE HEAD
Extend the possibility


ERGONOMICS DESIGN
optimize the hand-grip use

EXPERT IN LED CURING LIGHT
13 years professional technology, 39 patents, 7 Invention Patents
Global sales over 600,000 units !

BASIC DATA:

Power input	AC100v-240v 50hz/60hz
Light intensity	1000mw/cm ² ~2300mw/cm ²
Net weight	278g
Dimensions:	25mm×25mm×240mm

3 SECONDS FOR CURING Up to 1600mW/cm² HIGH INTENSITY

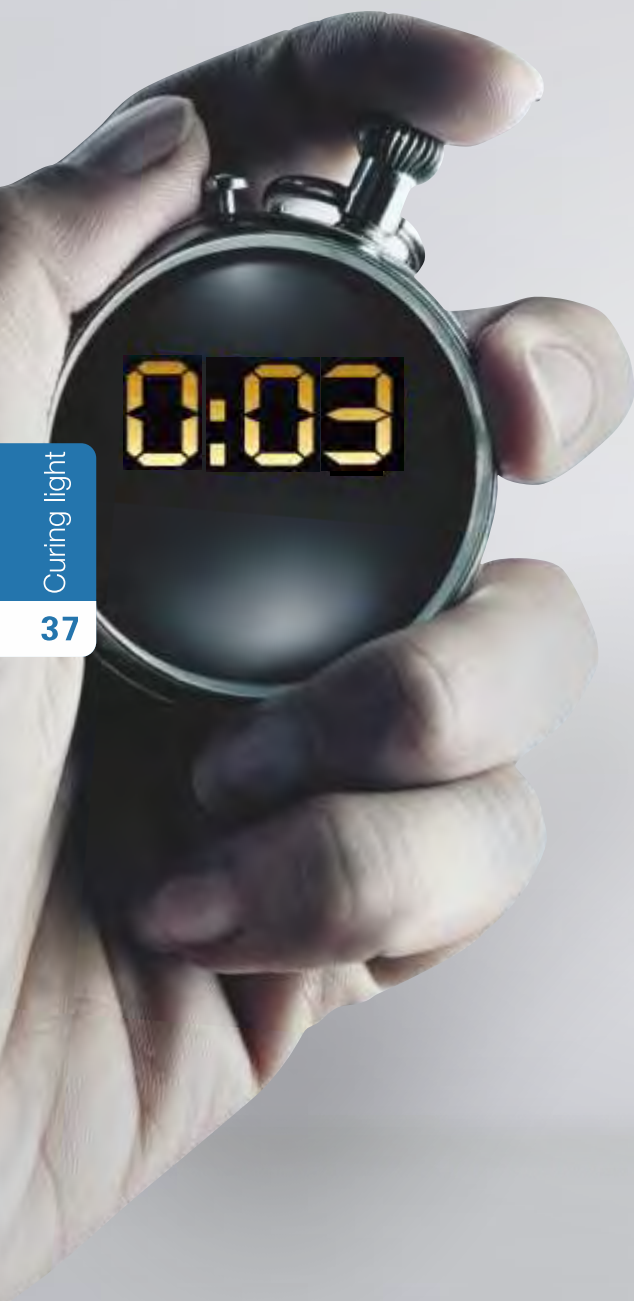

Curing light

37

LUX E

- Especially suitable to solidify agglomerant of orthodontic bracket, veneer and post.
- Wireless. The battery can be replaced.
- Three working modes: Low, Middle, High.
- Constant light intensity. The solidification effect is not affected by the consumption of remaning power.
- Large capacity battery. A full charge can be used for more than 400 times continuously under 10s working time mode.
- Low standby power consumption with 70 days' standby time.



Industrial design patent No.:CN 200930321063.7

Power input	AC100V to 240V 50Hz/60Hz
Light output	800mW/cm ² -1600mW/cm ²
Net weight	141g
Dimensions	260mmX40mmX50mm

LUX V

- Large capacity battery. A full charge can be used for more than 300 times continuously under 10s working time mode.
- Low standby power consumption with twenty days' standby time.
- Constant light intensity. The solidification effect is not affected by the consumption of remaining power.
- Power indicator.
- Suitable for both right or left hand operation.



Industrial design patent No.:CN 201130028451.3

Power input	AC100V to 240V 50Hz/60Hz
Light output	1000mW/cm ² -1200mW/cm ²
Net weight	85g
Dimensions	263mmX31mmX23.5mm

MINI S Curing light

- Woodpecker,High Quality Manufactured.
- Comfortable ergonomic design.
- Simple one-button operation.
- More than 300 times 10-second cures.
- Constant light intensity output.

NEW



Battery	3.7V/1400mAh
Dimensions	230mm×26mm×30mm
Power Input	~100V-240V 50Hz/60Hz
Power Output	4.2V \square 1A

Curing light

38

EXPERT IN LED CURING LIGHT !
14 years professional technology,
41 patents,8Invention Patents
Global sales over 600,000 units !

LUX VI

- Ergonomic design, small and convenient
- Special light hood and holder design, high-effectively filtering light
- Three working modes: Full, Ramping, Pulse.
- Time setting: 5s, 10s, 15s, 20s
- A full charge can be used for over 300 times. (10s/time)
- Constant light intensity, the solidification effect is not affected by the consumption of remaining power.
- With wire or wireless. It can run directly on commercial power supply whilst the battery runs out.



Optional colors



Industrial design patent No.: CN 201230421494.2

Power input	AC100V to 240V 50Hz/60Hz
Light output	1000mW/cm ² -1200mW/cm ²
Net weight	100g
Dimensions	234mmX26mmX26mm

LUX I

- 220 degrees head rotation.
- Disposable sleeve:Save autoclaving time.
- Easy-to-change battery.
- Automatic memory.Avoid setting frequently.
- Stable output of light intensity,the solidification effect is not affected by the consumption of remaining power.
- Efficient transfer from electricity into light.A full charge can be used more than 400 times continuously under 10s working time.

Industrial design patent No.:CN 201230045664.1

Power input	AC100V to 240V 50Hz/60Hz
Light output	850mW/cm ² -1000mW/cm ²
Net weight	230g
Dimensions	79.5mmX79.5mmX261mm



LED.H ORTHO

A TOUCH AND DONE, ALL FOR ORTHO.

Rapid orthodontic 3 seconds for curing

Intensity light 1,800mW/cm², only 3 seconds to solidify the bracket.

Beveled light guide

Easy to touch any part of teeth , Can radiate vertically at any angles , especially suitable for posterior teeth

Continuous work time

Full metal body for intelligent cooling system , preventing overheating after long-time work.



Power input	AC100V to 240V 50Hz/60Hz
Light output	1000mW/cm ² -1200mW/cm ²
Net weight	178g
Dimensions	252mmX25mmX25mm



KINGKONG series drop
Resistant dental handpiece

MORE POWERFUL AND MORE EFFICIENT

Thanks to the new optimized wind wheel and gas path design


Torque is up to **7.5gf.cm**, which has increased by **62.8%** compared to old type handpiece.

As a result, the cutting efficiency is increased by **94.6%**.

OVERLOAD PROTECTION SYSTEM



Feature article of overload protection system

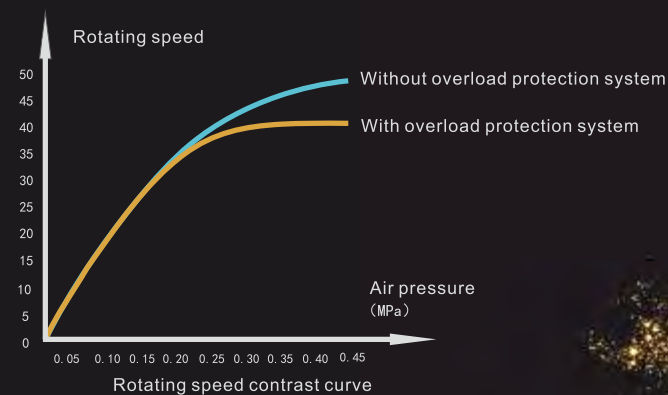

The new overload protection system can protect the handpiece from higher pressure, prolonging handpiece's life span.
Dentists do not need to frequently adjust the air pressure, which is more convenient and efficient.

AXIAL CORE WITH BIGGER CLAMPING FORCE



Pull to red graduation :16N
Pull to yellow graduation :20N
Pull to green graduation :24N

Non-spring structure axial core design

It has larger clamping force (which is up to 35N) compared to traditional spring structure axial core.


It can grasp the niddle tighter

It wouldn't be hard to uninstall the burs after intense cutting,
making it more convenient to install and uninstall the burs.

THE CHAMPION AMONG EXCELLENCES


Cutting force raises **94.6%**

HP 33

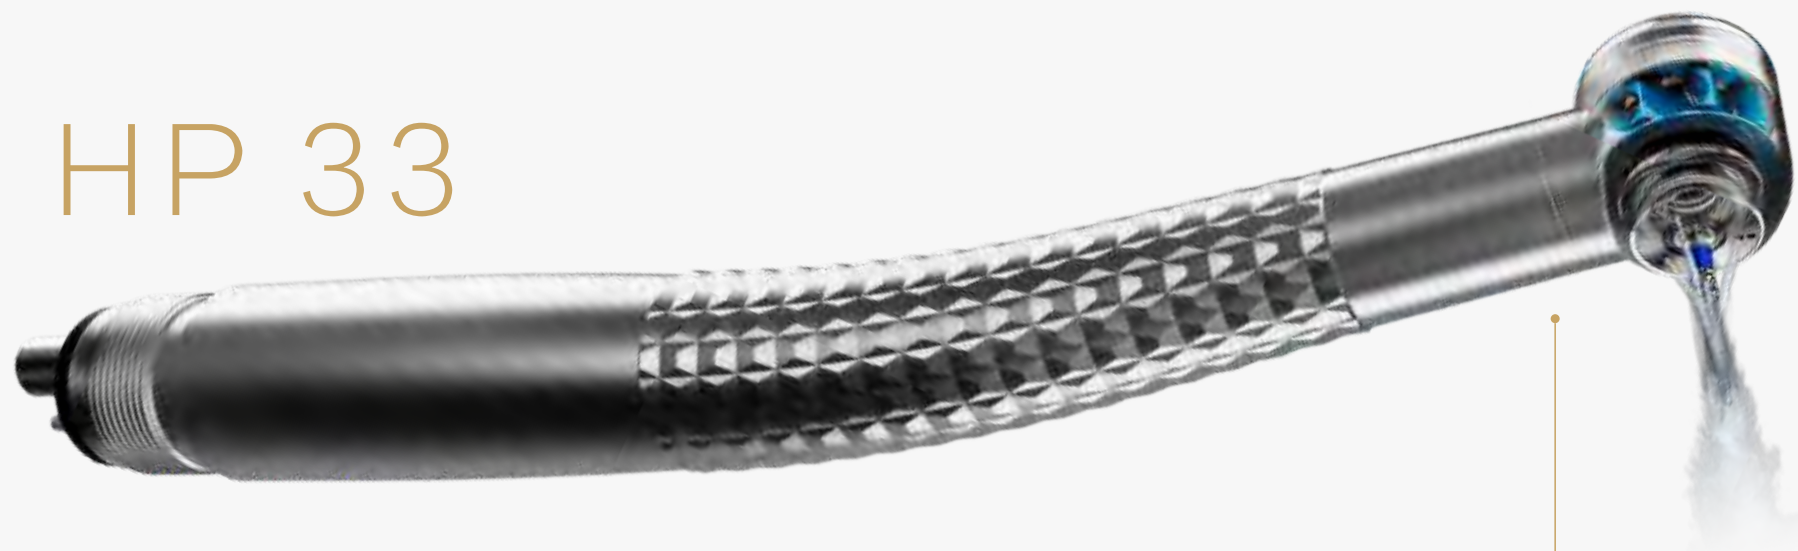

Anti-suction Sanitary Head System

Negative pressure tends to cause ingress of foreign substance such as flood and germs while the handpiece stopping rotating. Special wind wheel and head design prevents back suction whilst prevent foreign substance from getting into the core of machine, prolonging the service life of bearing.

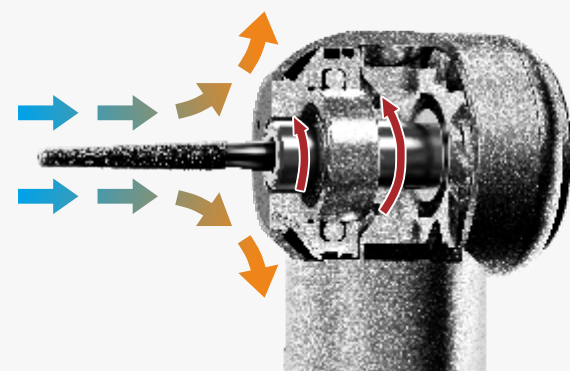


Strong enough clamping force Tighter needle grasping

Non-spring structure axial core design
Stronger clamping force (up to 35N) enables tighter needle grasping
It wouldn't be hard to remove after intense cutting,
making it more convenient to install and uninstall the burs.
The following figure shows three scales of clamping forces on the measuring tool
Pull to red graduation: 16N
Pull to yellow graduation: 20N
Pull to green graduation: 24N



Imported ceramic bearing

Wear-resistant cage enables longer service life.

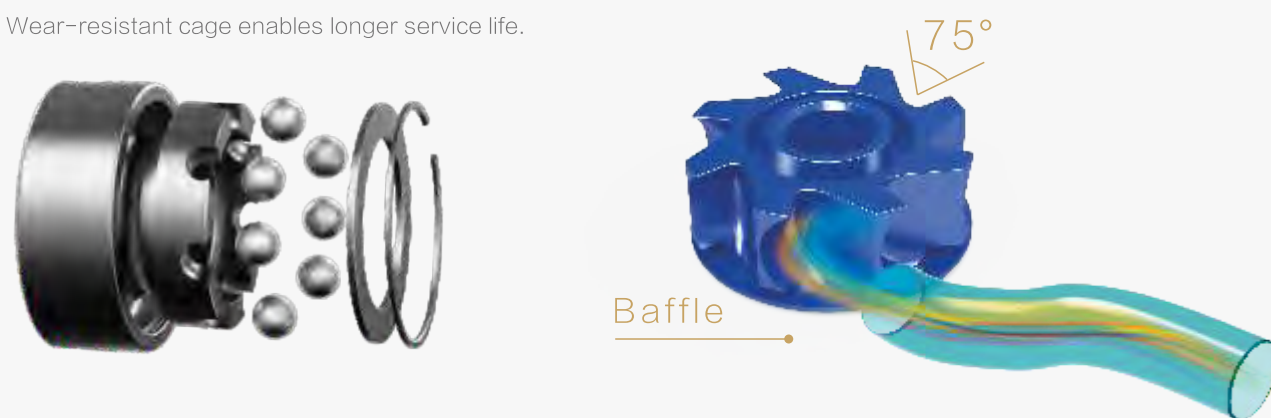

Three-hole atomization Better cooling effect

Traditional single-hole handpiece cannot completely cool down for the limit of flow and angle. Especially for the deep-hole cutting such as pulp exposing, as the angle is limited, the cutting area cannot be cooled, which will burn the teeth tissue. Three-hole atomization handpiece takes the burr as axis to spray atomized water to the treatment area from various angles, wrapping the burr, reducing the risk of burn the teeth tissue during cutting process.



Model	HP33-M4/B2	HP11-M4/B2	HL11-M4/B2
Type	Big head push type	Standard push type	Standard push type
Characteristics	Anti-suction system Single-hole atomization Strong cutting force	Small head with strong force Single-hole atomization Overload protection Tighter burr grasping	Standard head Single-hole atomization Strong cutting force Overload protection
Air pressure	0.25-0.27MPa	0.18-0.22MPa	0.18-0.22MPa
Water pressure	0.1-0.25MPa	0.1-0.25MPa	0.1-0.25MPa
Rotation speed	0.3-0.35 million rpm	0.36-0.43 million rpm	0.36-0.43 million rpm
Head height	13.4mm	13.1mm	12.0mm
Head diameter	Φ 12.0mm	Φ 11.2mm	Φ 11.2mm
Noise	< 70dB	< 70dB	< 70dB

SURGERY X

The Third Generation Woodpecker Ultrasurgery

Micron Cutting

The cutting power of Ultrasurgery is derived from micro-oscillation. The amplitude of tip is between 20–100 μ m. There is only micro-amplitude vibration that is invisible to the naked eye at the end of tip. The tip and bone tissue are in uniform contact with no bounce and smoother cutting, which increases controllability.

Ultrasurgery working accuracy is in micrometers. The minimum surgical incision is 3.5mm long, 0.5mm wide, which will help with small operating area and fast postoperative recovery.



7-inch Touching Screen

Abandoning the previous button operation settings, innovatively adopting 7-inch screen. While clearly displaying information, operate directly by tapping the screen.



Multi-function Foot Pedal

Multi-function foot pedal, makes it easy to control water flow, working mode, and power, simplifying operation procedures and realizing efficient operation.



Tips Kit

Specially used for tooth extraction, crest splitting, and retropreparation. Adopt gold plating which is wear-resistant and practical with long time of endurance.



DS-II LED

Woodpecker core technology, reliable cutting efficiency professor


38 patents, 9 invention patents

15 years of R&D, 29 years' Ultrasonic Technology Professor

Exported to 89 countries, including Germany, Switzerland, Italy etc.



Comparison of cutting efficiency with other famous brands

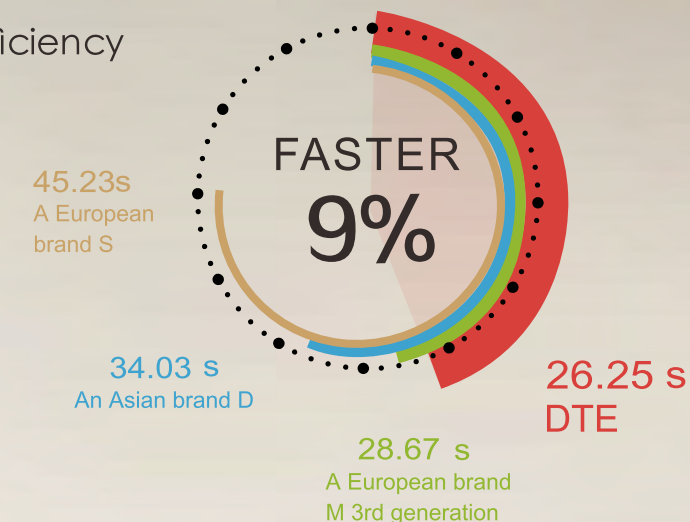


NEWLY DEVELOPED HANDPIECE

Developed internal Structure: handpiece and tip are more compatible, with steady output
Developed packaging technology: more stable after UHT sterilization, with constant quality


SAFE

Handpiece and pump line can burden UHT sterilization, to make sure the bacteria-free environment

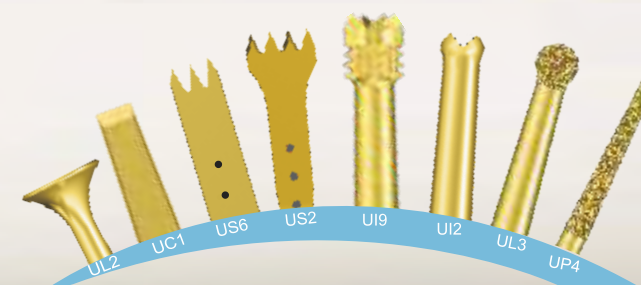

Micrometric cuts, Selective cuts,
No harm to soft tissue


Equipped with **×2**

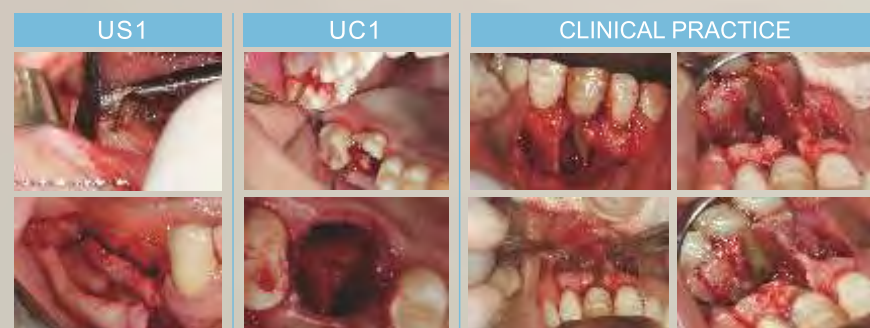

Technical parameters

Power input	100 - 240V ~ 50Hz/60Hz 600mA (max)
Frequency	24kHz ~ 36kHz
Power output	5W ~ 35W
Main unit weight	3.1kg
Dimensions	330mm × 254mm × 167mm


HIGHLIGHT LAMP
CLEAR VISIBILITY




DTE Brand **33°C**



Well-known European Brand S **30°C**



Well-known European Brand M **33°C**



Well-known Asian Brand D **38°C**

WORKING 10 MIN UNDER FULL POWER
TEST THE TEMPERATURE OF HANDPIECES








More powerful than you imagine

Please use the correct scaler tip

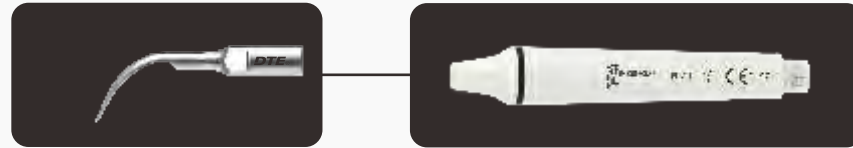Tips marked with **DTE** connected to handpiece marked with  will lead to serious problem.



Tips marked with  connected to handpiece marked with **DTE** will lead to the same problem.


 These kinds of damages are not covered under warranty.



The comparison between DTE tip and disposable tip made in China



DTE tip spray evenly, effective cleaning and cooling

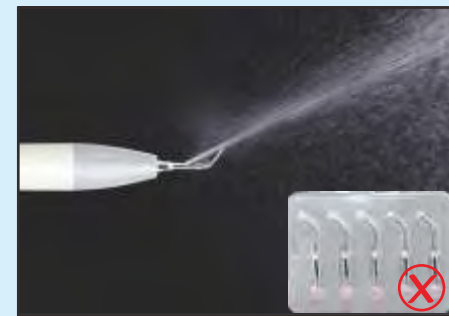

The water spray slanting more than 70% of disposable tip, unable to clean the teeth and cool the tip

The comparison between DTE tip and other tips made in China after sterilization



After 300 cycle sterilized, there isn't any rust on DTE tip, No crack after working 1000 hours



Tips of poor quality start to be cracked after one-hour working, the cracking rate within 10 hours is 35%.



After working 6 minutes, Tips of poor quality started to crack, after 12 hours, all the tips are cracked

If the cracked tip were swallowed by patients, it will cause serious medical accidents

To guarantee the safety of you and your patients, please choose original Woodpecker tip

Please choose authentic Woodpecker tips!
Reject to use disposable tips of poor quality!

Scaling

GD1

Supragingival scaling

GD2

Supragingival scaling

GD3

Supragingival scaling

GD4

Supragingival scaling

GD5

Supragingival scaling

GD6

Supragingival scaling

GD7

Remove dental crown

GD8

Remove dental pile, with irrigation

GD9

Supragingival scaling

GD10

Supragingival scaling

GD11

Orthodontic treatment

Periodontics

PD1

Periodontal scaling

PD3

Periodontal scaling

PD4

Periodontal scaling

PD3D

Smoothing restoration overhangs and debride in-depth root (diamond-coated)

PD2L

Periodontal scaling

PD2R

Periodontal scaling

PD2LD

Remove calculus from narrow inter-root spaces (diamond-coated)

PD2RD

Remove calculus from narrow inter-root spaces (diamond-coated)

Cavity preparation

SBD1

Removing the caries on occlusal surface of teeth and dental neck

SBD2

Removing the caries on Mesial surface of the adjacent teeth

SBD3

Removing the caries on Distal surface of the adjacent teeth

GD31

Preparation of mesiocclusion cavity

GD33

Preparation of teeth veneer

SBDL

Half ball diamond tip. Set 45° to the left, to remove the carious teeth without damaging the adjacent teeth.

SBDL

Half ball diamond tip. Set 45° to the right, to remove the carious teeth without damaging the adjacent teeth.

GD30

Preparation between pits and fissures

GD32

Preparation of distal and mesial cavity

Shoulder preparation

GD20

Abrade dentin

GD21

Fine repair and polish the prepared shoulder

Endodontics

ED1

120°angle holder, for root canal cleaning

ED2

95°angle holder, for root canal cleaning

ED3

For the lateral thermal condensation of gutta-percha

ED3D

Used to remove the calcification and bad filling material of pulp cavity (diamond-coated)

PD4D

Remove calcification in the coronal third of the root canal (diamond-coated)

ED4

Remove obstructions and broken instruments in the root canal

ED4D

For retreatments and remove hard materias (diamond-coated)

ED5

Remove root canal fillings and broken instruments in the coronal third

ED5D

Remove dental overhangs in the pulp chamber (diamond-coated)

ED8

Burs holder, used to expand root canal and grind teeth

ED9

Burs holder, used to expand root canal and grind teeth

ED10

Used for root canal softly treatment

ED10D

Used for root canal retrogression, efficient root apical polishing (diamond-coated)

ED11

Used for root canal softly treatment

ED11D

Used for root canal retrogression, efficient root apical polishing (diamond-coated)

ED14

Remove obstructions and broken instruments in the root canal, with irrigation

ED15

Remove root canal fillings and broken instruments in the coronal third, with irrigation

ED14D

Remove calcification in root canal, root canal cleaning and enlargement

ED15D

Remove calcification in root canal, root canal cleaning and enlargement

NITI K-File



15# 20# 25# 30# 35# 40#

Tip with excellent tenacity is used for root canal cleaning
File size: 32.5mm±0.5mm
Handpiece size: Φ0.68mm~0.71mm
K-file taper: 2%
Each kit with six pieces, one kit for one model

Scaling

GD1T

Supragingival scaling

GD2T

Supragingival scaling

GD3T

Supragingival scaling

GD4T

Supragingival scaling

GD5T

Supragingival scaling

GD6T

Supragingival scaling

GD7T

Remove dental crown

GD8T

Remove dental pile, with irrigation

GD9T

Supragingival scaling

GD10T

Supragingival scaling

Endodontics

ED1T

120°angle holder, for root canal cleaning

ED2T

95°angle holder, for root canal cleaning

ED3T

For the lateral thermal condensation of gutta-percha

ED4T

Remove obstructions and broken instruments in the root canal

ED5T

Remove root canal fillings and broken instruments in the coronal third

ED8T

Burs holder, used to expand root canal and grind teeth

ED9T

Burs holder, used to expand root canal and grind teeth

ED10T

Used for root canal softly treatment

ED11T

Used for root canal softly treatment

ED14T

Remove obstructions and broken instruments in the root canal, with irrigation

ED15T

Remove root canal fillings and broken instruments in the coronal third, with irrigation

Periodontics new

PD1T

Periodontal scaling

PD2LT

Periodontal scaling

PD2RT

Periodontal scaling

PD3T

Periodontal scaling

PD3LT

Periodontal scaling

PD3RT

Periodontal scaling

PD4T

Periodontal scaling

PD5T

Periodontal scaling

PD10T

Periodontal scaling

PD11T

Periodontal scaling

PD12T

Periodontal scaling

PD14LT

Periodontal scaling

PD14RT

Periodontal scaling

PD18T

Periodontal scaling

PD20T

Periodontal scaling

PD20LT

Periodontal scaling

PD20RT

Periodontal scaling

PD21LT

Periodontal scaling

PD21RT

Periodontal scaling

PD22LT

Periodontal scaling

PD22RT

Periodontal scaling

Bone surgery

US1

Osteotomy

US1L

Osteotomy

US1R

Osteotomy

US2

Osteotomy

US3

Osteotomy of precision in the thin regions

US4

Bone remodeling and bone chip harvesting

US5

Bone remodeling and bone chip harvesting

US6

Precise osteotomy

Sinus lifting

UL1

120° Peeling of the sinus membrane

UL2

Peeling of the sinus membrane

UL3

Non-traumatic bone cutting on thin bone region (diamond-coated)

UL4

Micrometric osteotomy near the soft tissue (diamond-coated)*The size of diamond grit is 100µm.

UL6

Peeling of the sinus membrane (angle: 95°)

Endodontic

UE1

Apical root debridement (diamond-coated) *The size of diamond grit is 40µm.

UE2

Soft apical root debridement

UE3

Apical root debridement (diamond-coated) *The size of diamond grit is 40µm.

UE4

Soft apical root debridement

Exelcymosis

UC1

Used for cutting ligaments, minimally damnification exelcymosis

UC3

Used for cutting ligaments, minimally damnification exelcymosis

UC2

Used for cutting ligaments, minimally damnification exelcymosis

Implantation

UI1

Used for implant, with tip ball Φ 1.6mm

UI2

Used for implant, with tip ball Φ 2mm, irrigation from tip point

UI3

Φ 2mm implant site preparation tip, irrigation from tip point.

UI4

Φ 3mm implant site preparation tip, irrigation from tip point.

UI5

Φ 2mm implant site preparation tip, irrigation from tip point.

UI6

Φ 3mm implant site preparation tip, irrigation from tip point.

UI7

Finalize the implant site and bone preparation (diamond-coated)

UI8

For implantation, in plus size, with tip ball Φ 1.6mm

UI9

Used for implant, with tip ball Φ 2.8mm

Periodontal surgery

UP1

Root scaling

UP2

Root scaling

UP3

Root scaling

UP4

Root surface debridement and root planning (diamond-coated)
*The size of diamond grit is 40 μ m.

UP5

Perio treatment

UP6

Bone remodeling, root planing in perio operation *The size of diamond grit is 40 μ m.

UP7

Bone remodeling and root canal enlargement (diamond-coated)
*The size of diamond grit is 40 μ m.

Scaling (Used for SIRONA)

GS1

Supragingival scaling

GS2

Supragingival scaling

GS3

Supragingival scaling

GS4

Supragingival scaling

GS5

Supragingival scaling

GS6

Supragingival scaling

GS7

Remove dental crown

GS8

Remove dental pile, with irrigation

Endodontics (Used for SIRONA)

ES1

120°angle holder, for root canal cleaning

ES2

95°angle holder, for root canal cleaning

ES3

For the lateral thermal condensation of gutta-percha

ES3D

Used to remove the calcification and bad filling material of pulp cavity (diamond-coated)

PS4D

Remove calcification in the coronal third of the root canal (diamond-coated)

ES4

Remove obstructions and broken instruments in the root canal

ES5

Remove root canal fillings and broken instruments in the coronal third

ES8

Burs holder, used to expand root canal and grind teeth

ES10

Used for root canal softly treatment

ES11

Used for root canal softly treatment

ES14

Remove obstructions and broken instruments in the root canal, with irrigation

ES15

Remove root canal fillings and broken instruments in the coronal third, with irrigation

DS-II LED Tip Series

A Wide Choice for Application

Basic kit

Sinus lift kit

Osteotomy kit

Extraction kit




Periodontal kit

Retro surgical kit

Implant prep kit

Periodontics (Used for SIRONA)

PS1






Periodontal scaling

PS3



Periodontal scaling

PS4



Periodontal scaling




PS3D



Smoothing restoration overhangs and debride in-depth root (diamond-coated)

Scaling (Used for KAVO)

GK1



Supragingival and subgingival scaling

GK2





Supragingival and subgingival scaling

GK3






Supragingival and subgingival scaling

GK4






Supragingival and subgingival scaling

GK5



Supragingival and subgingival scaling

GK6



Supragingival and subgingival scaling

GK7






Supragingival and subgingival scaling

GK11






Orthodontic treatment

GC1



Supragingival and subgingival scaling

GC2



Supragingival and subgingival scaling

EK8



Burs holder, used to expand root canal and grind teeth

Periodontics (Used for KAVO)

PC1



Subgingival scaling

Used for AMDENT

A1






Supragingival scaling

A2



Supragingival scaling

A1T



Supragingival scaling

HD-8L

Used for :DTE scaler with detachable handpiece. With light, better view, autoclavable. Complete metal-made body



Weight	62.33g
Dimensions	114.36mm x Φ19.1mm

HD-8H

· USED FOR: DTE scalers with detachable handpiece. without light



Weight	56g
Dimensions	123mm×Φ20.5mm

HD-7L

· USED FOR: DTE scalers with detachable handpiece, with light, better view, autoclavable. Plastic head and metal head are optional.



Weight	63g
Dimensions	111mm×Φ20.5mm



Weight	57g
Dimensions	111mm×Φ20.5mm

HD-7H

· USED FOR: DTE scalers with detachable handpiece, without light , autoclavable.
· Two colours optional (white/ blue)



Weight	57g
Dimensions	117mm×Φ21mm



Weight	57g
Dimensions	117mm×Φ21mm

HD-2L New!

· USED FOR: D2 LED, with light , better view,handpiece sleeve is autoclavable
· Three colours optional to the handpiece sleeve (green/ blue/ amethyst).





Weight	156g (+cable)
Dimensions	140mm×Φ20mm

HD-1

· USED FOR: D1/V1.



Weight	124g (+cable)
Dimensions	125.7mm×Φ18mm

Spare parts for ultrasonic scaler

AT-1
Auto water supply system

- Instead of infusion bottle, it can be placed at any flat surfaces to fit the working environment.
- Made of high-qualified material, it is safe and durable.
- Pneumatic water control ensures consistency in water pressure.
- Compatible with scalers of any brands.
- Delicate in design, small in space occupation.



Autoclavable set
Handpiece×1
Torque wrench×1
Endo wrench×1
(6 tips optional)

Detachable cable
With different connectors,
available for handpiece
HD-7H, HD-7L respectively

TD-1L Torque wrench
← Hold the tips.
TD-1 Torque wrench
← Can not hold
the tips.

TD-2L Torque wrench
Hold the tips.

TD-E1 Endo wrench
Used for changing the
ultrasonic U-file and
screwing / unscrewing
the endo chuck
TD-A wrench
For replacement of dental
burs and burs holder

TD-5L Torque wrench
For DTE and SATELEC
scaler tips
TS-5L Torque wrench
For Sirona scaler tips
TK-5L Torque wrench
For Kavo scaler tips

TW-3 Wrench

Peristaltic pump

1# Tip holder

2# Tip holder

Foot switch(round)

LED lamp

File stand

Foot switch(square)

Quick connector

Diaphragm pump

Spare parts for dental turbine handpiece

HL11-M4/B2
Cartridge

HP13-M4/B2
Cartridge

HP11-M4/B2
Cartridge

HL13-M4/B2
Cartridge

Bur key

Bearing A
(steel ball)

Cap spanner applicable
for HP13-M4/B2
HL11-M4/B2

Cap spanner applicable
for HL11-M4/B2

Cap spanner applicable
for HL13-M4/B2

Cap spanner applicable
for HP11-M4/B2

Spare parts for apex locator

Lip hook

Measuring wire

File clip

Measuring file

Tester

Endo ruler

Spare parts for curing light

Optical fiber
Black and white optional
Can be autoclaved under high
temperature and high pressure
1# Dimensions: Φ8mm
2# Dimensions: Φ8mm
1# Applicable for: LUX E
2# Applicable for: LUX V、LUX VI

For LUX I、LUX E For LUX V、LUX VI
Adapter
Power input:
AC100V-240V 50Hz/60Hz
Output voltage/current:
DC 5.0V/1.0A

1# 2# 3#
Light hood

① ② ③
Battery
①: ICR14500
Battery Voltage: 3.7V
Applicable for: LUX V、LUX VI
②: ICR18490A
Battery Voltage: 3.7V
Applicable fo LUX E
③: ICR18490B
Battery Voltage: 3.7V
Applicable for: LUX I

Lightmeter

Bathymeter

Disposable sleeve
for LUX I

LED lamp
3W、5W

Glasses