


Y-Adapter




For reprocessing instructions in accordance with ISO 17664 see www.duerrdental.com, order no: A700100009

For reprocessing instructions in accordance with FDA Guidance "Reprocessing Medical Devices in Health Care Settings - Validation Methods and Labeling" see www.airtechniques.com, order no.: A700100008

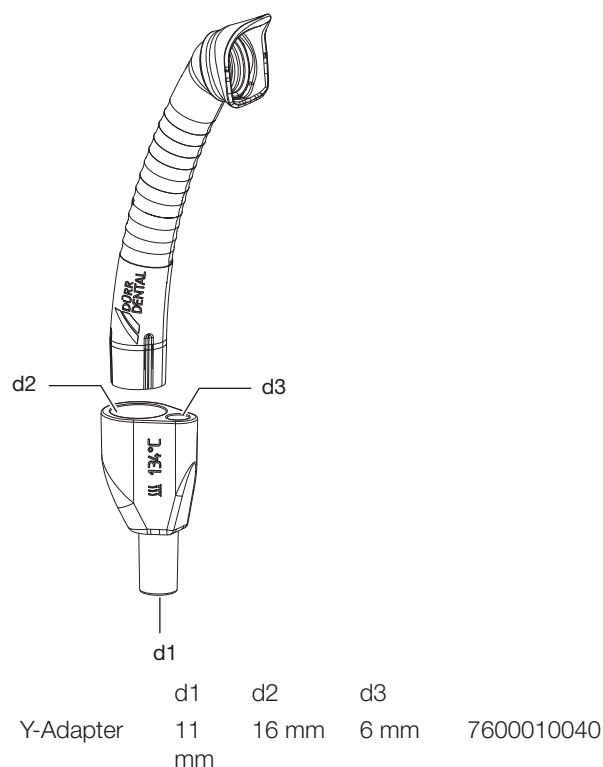

Aerosol reduction

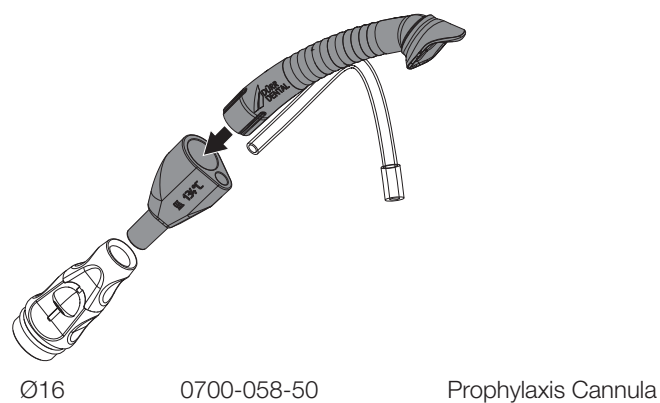

Adapter from 11 mm to 16 mm

